

Republic of the Philippines
Department of the Interior and Local Government
NATIONAL POLICE COMMISSION
DILG NAPOLCOM Center
EDSA cor. Quezon Avenue,
West Triangle, Quezon City

RESOLUTION NO. 2017-510

APPROVING THE PNP-UESB RESOLUTION NO. 2016-089 DATED JUNE 15, 2016
THAT PRESCRIBES THE MINIMUM STANDARD SPECIFICATIONS FOR
INFUSION PUMP

WHEREAS, Section 14, Paragraphs (i) and (m) of Republic Act No. 6975 as amended by Section 5, Sub-Paragraphs (5) and (8) of the Republic Act No. 8551, empowers the Commission to “approve or modify plans and programs on education and training, logistical requirements, communications, records, information system, crime laboratory, crime prevention and crime reporting as well as prescribe minimum standards for arms, equipment and uniforms and, after consultation with the Philippine Heraldry Commission, for insignia of ranks, awards and medals of honor;”

WHEREAS, pursuant to the aforesaid legal prescription, the PNP, through its Uniform and Equipment Standardization Board (UESB) Resolution No. 2016-089 dated June 15, 2016, has favorably submitted and indorsed the proposed minimum standard specifications for Infusion Pump, for consideration/approval of the Commission;

WHEREAS, the PNP UESB subject proposed specifications refers to the descriptions and parameters requirements of Infusion Pump as a medical device that delivers fluids, such as nutrients and medications, into a patient’s body in controlled amounts which is intended to be used in the Philippine National Police General Hospital (PNPGH) particularly in the Intensive Care Unit (ICU) to enhance the capability of health care management;

WHEREAS, the PNP Directorate for Research and Development (DRD) certified the proposed subject minimum standard specifications as contained in the UESB resolution are not a tailored-fit specification to any particular brand of product in the market;


WHEREAS, upon thorough review and evaluation, the Commission has determined that the herein proposed minimum standard specifications for Pulse Monitor (Pulse Oximeter) are in order and conform with the requirements of Republic Act No. 6975, as amended by Republic Act No. 8551, its Implementing Rules and Regulations (IRR), logistics policies and issuances of the Commission, to meet the requirements of the PNP;



NOW THEREFORE, the Commission, in the exercise of its statutory powers to administer and control the PNP, HAS RESOLVED, AS IT HEREBY RESOLVES TO APPROVE the minimum standard specifications for Infusion Pump, with modifications to read as follows:

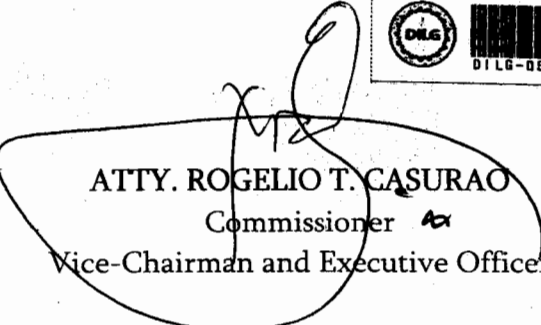
- | | | |
|-----------------|---|-----------------|
| 1) Flow Range | : | 0.1 – 999.9ml/h |
| 2) Volume Limit | : | Up to 9999ml |
| 3) Accuracy | : | ±5% |

- | | | |
|---------------------------|---|--|
| 4) Display | : | FND 7 or LCD |
| 5) Occlusion Detector | : | Capable to detect occlusion at 15kPa |
| 6) Alarms | : | Occlusion
Malfunction
Low battery
Bubbles in the tube |
| 7) Power Source | : | AC/DC |
| 8) Battery | : | Rechargeable |
| 9) Waterproof | : | IPX1 |
| 10) Weight | : | 2.5 kg maximum |
| 11) Operating Temperature | : | 5°C to 40°C |

APPROVED this 11th day of OCTOBER 2017 in Quezon City, Metro Manila, Philippines.

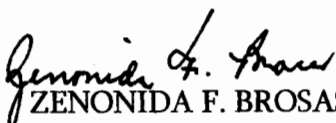

CATANNO S. CUY
 Officer-In-Charge
 Office of the Chairman, NAPOLCOM

 
 DILG-DBEC 01012018-13834


ATTY. ROGELIO T. CASURAO
 Commissioner
 Vice-Chairman and Executive Officer



FELIZARDO M. SERAPIO, JR.
 Commissioner


JOB M. MANGENTE
 Commissioner


ZENONIDA F. BROSAS
 Commissioner


RONALD M. DELA ROSA
 Ex-Officio Commissioner

Attested by:


ELVIRA M. BAUTISTA
 Acting Chief, Secretariat